

2 & 3 DIVER RAPID DEPLOYMENT CONSOLE MAINTENANCE MANUAL



Dive Lab, Inc.

1415 Moylan Road, Panama City Beach, FL 32413 Phone: 850-235-2715 Fax: 850-235-0858 E-mail: divelab@divelab.com

Definitions of Signal Words Used in this User's Guide

DANGER

This word indicates an imminently hazardous situation, which if not avoided, will result in death or serious injury.

WARNING

This word indicates a potentially hazardous situation, which if not avoided, could result in death or serious injury.

CAUTION

This word indicates a potentially hazardous situation, which if not avoided, may result in minor or moderate injury. It may also be used to alert against unsafe practices.

NOTICE

This word indicates a special attention or required action for basic operation.

TABLE OF CONTENTS

SECTION ONE: GENERAL INFORMATION	PAGES
Definitions	1
Advantages	1
User Guide	2
Foundation Plate Screws	2
Cleanliness	2
Shut Down	2
SECTION TWO: CONCEPT AND INTENDED USE	
Conventional Surface Supplied Diving	3
RDC-2 & RDC-3 Major Subsystems	3
High Pressure Supply	3-4
SECTION THREE: CONFIGURATION AND USE	
Rapid Deployment Air Control Console (RDC)	5
RDC-3 Specifications	6
High Pressure Air System	6
SECTION FOUR A: REPAIR, MAINTENANCE & OVERHAUL PROCEDURES	
General Cleaning / Inspection Procedures	7
Pipe Threads	7-8
Checking & Quantifying Leaks	8-9
Torque Tightening	9
RDC Regulator	9-13
Low Pressure Umbilical Supply Valves/Cross-Connect Valves	13-17
Check Valve/One-Way Valve	17-20
Pneumofathometer Valve Lubrication	20-21
High Pressure Supply Valve	22-24
Relief Valve	24-27
Hylock SS Angle Relief Overhaul	27-29
SECTION FOUR B: REPAIR, MAINTENANCE & OVERHAUL PROCEDURES	
RDC System Pressure Gauge Comparison	30
RDC System Pressure Test Procedure	30-31
RDC Annual Relief Valve Lift Check	31-32
SUPPLEMENTAL INFORMATION	
Exploded View for Aqua Environment Regulator	33
RDC/XLDS O-Ring Chart	34

SECTION ONE: GENERAL INFORMATION

GENERAL INFORMATION

The Rapid Deployment Console RDC was originally designed and engineered by Dive Lab, Inc., to supply a complete surface supply system known as the Extreme Lightweight Diving System (XLDS).

The XLDS system consists of the RDC, HP supply system, lightweight umbilicals and Intermediate compensating system with diver worn harness and EGS system. The XLDS was primarily designed for Military and public safety diver use. The RDC is available in two models, the RDC-2 (2 diver) and RDC-3 (3 diver) consoles

This Maintenance Manual covers both the two and three diver RDC's consoles "only" for use with convention surface supply diving techniques. There will be reference to the XLDS.

DEFINITIONS

RDC-2: Rapid deployment, 2 Diver Control Console

RDC-3: Rapid Deployment, 3 Diver Control Console

XLDS: Extreme Lightweight Diving System

ICS: Intermediate Compensating System

SCUBA: Self Contained Underwater Breathing Apparatus

UMBILICAL: Consists of air, communications/strength member and Pneumofathometer hose that supports the diver

HIGH PRESSURE: Pressure supplying the reducing regulators usually above 400 PSIG

LOW PRESSURE: The air being supplied to the reduced pressure circuit, normally 325-375 PSIG for the intermediate system, and up to 250

PSIG for conventional surface supplied diving using 3/8" Umbilicals

PNEUMO QD: Pneumofathometer Quick Connect

OB: Over Bottom

PSIG: Pounds per Square Inch Gauge pressure

PSIG OB: Pounds per Square Inch Over the Bottom pressure

RMV: Respiratory Minute Volume

WOB: Work Of Breathing

EGS: Emergency Gas System

LPM: Litres Per Minute

FSW: Feet Salt Water

FFW: Feet Fresh Water

RMV: Respiratory Minute Volume

BPM: Breaths Per Minute

SSOCS: Surface Supplied Oxygen Control System

ADVANTAGES OF THE RDC

- Lightweight highly portable
- Low maintenance

For conventional surface supplied air diving, both the 2 and 3 diver Rapid Deployment Console RDC, and HP supply may be used with many conventional helmets and full-face masks providing the maximum flow and pressure requirements are met.


SECTION ONE: GENERAL INFORMATION

THE USER GUIDE

Whenever the XLDS is referred to in this user guide, it refers to the entire system. However, both the 2 and 3 diver RDC units can also be used for conventional surface supplied diving using standard 3/8" (9mm) I.D. umbilicals.

FOUNDATION PLATE SCREWS

The RDC main foundation plate has nine (9) ¼-20 screws with nylon lock nuts that join the foundation plate to the case enclosure. These nine screws pass through soft silicone donut type shock mounts designed to allow the foundation plate to shift, and move, as the case is banged around. **IMPORTANT! Do not over tighten these screws!** It is normal for the screws to be loose, so that the foundation plate which holds the manifolds can absorb shock and impact. The Nylock nuts do not allow the screws to loosen.

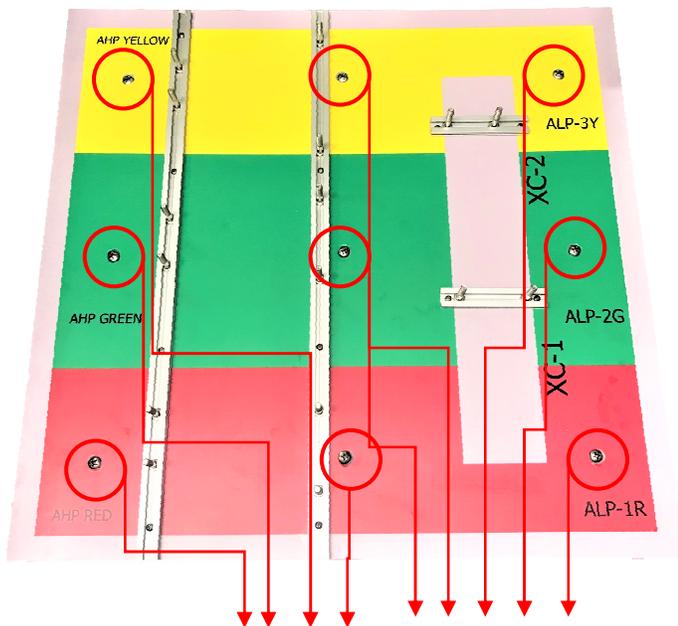

IMPORTANT! Do not over tighten these screws!

CLEANLINESS

Keep the interior of the RDC clean and wiped down. Wiping down the interior components with a solution of mild dish detergent and water will minimize corrosion and keep the system looking good.

SHUT DOWN

When the console is being shut down, ensure all pressure has been vented and all valves are shut. Keep inlet and outlet ports capped whenever the system is not in use. The same for all umbilical connections.

Ensure comm box is removed before console is closed for storage.

When closing the lid of the console box make sure you push in on the spring latch as shown below.



Detailed instructions of shut down procedure is found in Section Five, OP-4 Post Dive/Shutdown & Inspection.

SECTION TWO: CONCEPT AND INTENDED USE

Conventional Surface Supplied Diving

The “Rapid Deployment” air control consoles (RDC-2 and RDC-3) can be used as conventional air control console, surface supplied diving, with Helmets, full-face masks, and standard 3/8” umbilicals. For normal surface supply umbilical diving, the console will be used to maintain over bottom supply pressure normally no more than 250 PSIG OB. When the RDC-2 or RDC-3 consoles are used in this manner for conventional air diving, supply pressure can be regulated to each individual diver, IAW the operational pressure and supply requirements, dictated by the UBA being used, and IAW the recommended performance specifications as outlined in this user guide. When using with conventional 3/8” umbilicals, the RDC relief valves are normally set to relieve between 275-300 psig.

Currently the RDC-2 and RDC-3, are certified by Dive Lab, for use with all properly maintained current production models of KMDSI Band Masks, Helmets, and Full-Face Masks properly configured for conventional surface supplied diving. Other equipment may be used, contact Dive Lab for additional information.

RDC-2 & RDC-3 Major Subsystems

Both the RDC-2 and RDC-3 share the same basic subsystems and components laid out in a similar fashion. These include:

- High Pressure Supply System
- Rapid Deployment Control Console (RDC)

DANGER

All Divers using the surface supply equipment and associated man worn equipment, must be medically fit. All users must have a current diving medical exam, by a physician knowledgeable in the requirements of diving physicals.

DANGER

Only persons properly trained in the practice of surface supplied diving and surface supplied diving operations should use this equipment. Failure to have proper training and experience could result in injury or death.

DANGER

The XLDS-RDC-2, and XLDS-RDC-3 high-pressure systems, **should not** be used with pure oxygen, or oxygen enriched breathing gases, with an oxygen percentage greater than 21% by volume. Use of oxygen or oxygen enriched breathing gases in the high-pressure systems, may result in fire or explosion, resulting in serious injury or death.

High Pressure Supply


The High-Pressure Supply System is for air diving only, and is not designed or intended for breathing gases with an oxygen content greater than 21% oxygen by volume however the system has provisions for integration of pure oxygen or oxygen enriched gas for in water decompression, using a separate Dive Lab system known as the Surface Supply Oxygen Control Console System (SSOCS). The SSOCS that can be interfaced with the reduced pressure Manifold. The oxygen system is intended for use to a maximum depth of 50 FSW, for decompression purposes only.

SECTION TWO: CONCEPT AND INTENDED USE

The HP air supply system is rated for up to 5000 psig service with properly rated fittings. The HP system should only be supplied with breathing quality air via sources at supply pressures of 400 PSIG or greater capable of supplying at least 500 LPM. Typical air supply sources include standard single or double SCUBA Cylinders, Fire Fighting Cylinders, and/or any high-pressure supply up to 4350 psig, if DIN fittings are in use.

The standard High-Pressure Air Supply System for both the RDC-2 and RDC-3 for each diver circuit consists of two SCUBA “A” Yokes / DIN combination connections with Bleed Valves, and short (24”whips). Each set of Yokes /DIN sends air via the short Whips, to an isolation valve on a small manifold block used for supply, isolation and air switching. From the Junction Block air travels via a 6’ to 25’ long whip, to the console pressure regulators. On the RDC-3 the third diver (Yellow Diver), is the standby.

Each HP supply assembly quickly connects to the Regulator Inlets through the use of 72” long whips. Other configurations of supply whips and fittings are available. The flow capability of the high-pressure system, enables standard SCUBA Cylinders, to be used as low as 380 PSIG, before Cylinder switch-out is necessary. Other supply whips and configurations, can be used, providing they can provide the proper volume.

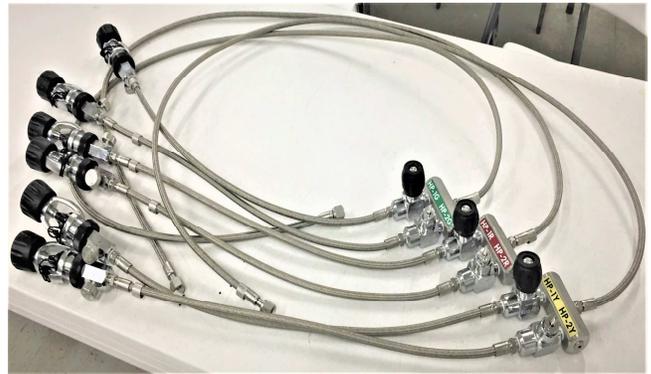

Typical High Pressure Assemblies



Special Purpose High Pressure Assembly



High Pressure Assembly with Gas Storage Cylinders

SECTION THREE: CONFIGURATION AND USE

Rapid Deployment Air Control Console (RDC)

The breathing gas control console regulates and controls the divers breathing air as well as pneumofathometer air for depth sensing. Both the two and three diver consoles (RDC-2, RDC-3), have one complete circuit for each diver laid out in a simple fashion, and the components used in each console, are the same. The Supply to each diver's circuit, starts with a VCO O-ring fitting, or # 4 37° JIC fitting, attached to a stainless-steel Street "T", connected to each diver's pressure regulator. The regulator is rated for a maximum inlet supply pressure of 5000 PSIG, and a maximum outlet pressure of 400 PSIG. Reduced air pressure passes through a one-way valve, allowing air to only travel into the Manifold. Each manifold assembly contains a 0-400 PSIG, reduced pressure gauge, Pneumofathometer supply valve, adjustable relief valve (set to relieve between 275-300 psig), and diver umbilical supply valve. Each manifold has a 1/2"-20, and 3/8"-28 straight thread gauge calibration ports, and a main supply cross connect, which allows intermediate air from either circuit, to be lined up to the other divers reduced pressure circuit(s). Each diver's air low-pressure (ALP) supply valves, are quick acting quarter turn valves. The manifold is the foundation, that holds all gas train components, and is secured to a 1/2" thick high-density polyethylene plastic foundation plate, that is through bolted to the console box, making the piping system secure.

The pneumofathometer gauges on the 2 and 3 Diver Console, are mounted in the console lid, along with or without an installed diver intercom (Optional). The 3 Diver Console can be equipped with several different diver intercom units (optional), but does not have a diver intercom integrated into box. Both 2 and 3 RDC's are

normally equipped with index locking quick connect fittings, for attaching the pneumofathometer and breathing air supply Umbilicals.

The RDC-2 or 3 can be used for air diving to a maximum diving depth of 220 fsw. The system must only be operated and used within the guidelines of this user guide, and the operation specifications described in this guide. The RDC-2 and 3 should not be used with oxygen enriched gas greater than 22% oxygen.



XLDS RDC-3

XLDS RDC-2



Pneumo attachment

SECTION THREE: CONFIGURATION AND USE

RDC-3 Specifications

- Box Weight 87 lbs.
- Outer Dimensions Length 28 inches
- Width 27 inches
- Height 15 inches
- Number Diver Circuits 3, Red, Green, Yellow
- Max Air Depth: Using 3/8" umbilicals 220 FSW
- Maximum High Pressure Supply 5000 Psig. With appropriate fittings
- Console Outlet Supply Pressure 0-400 psig
- Low Pressure Relief Setting: 275-285 psig
- High Pressure Gauges: 3, 0-6000 psig
- Low pressure Gauges: 3, 0-400 psig
- Pneumofathometer Gauges: 3, 0-250 fsw

High Pressure Air System

The standard high-pressure air attachment to SCUBA cylinders, are either DIN or SCUBA "A" Yokes, rated for a maximum supply pressure of (4350 psig DIN), (3500 psig A-Yoke). All standard RDC-2 and RDC-3 Whips, are rated for a maximum working pressure of 5000 psig, or as marked on the Whip. Other Whips up to 25 feet in length, can be used, providing they have a minimum I.D. of 0.112. Whips over 25 feet in length, should have a minimum I.D. of 0.160.



DIN Yoke Assembly

WARNING


The HP whips supplied are rated for 5000 psig service, but should not be used at pressures greater than 3500 psig, with the "A" Yoke or 4350 PSIG with DIN fittings, but can be used up to 5000 PSIG with other properly rated fittings.

CAUTION

Ensure the Cylinder Valve Outlet opening is pointing away, in a safe direction, then slightly crack open and shut each Cylinder Valve momentarily, to dispel any dust or dirt that may be present in the Valve Orifice.

Each divers' circuit comes standard, with two cylinder attachment whips and yokes, which attach to a routing block and shut-off valves. Each supply system allows attachment, to two single SCUBA cylinders, or two sets of twin SCUBA cylinders, if twin cylinders are being used. Each divers' circuit should always be set-up with each yoke or DIN attached to a fully charged cylinder, and only one cylinder should be on line at a time, so that when the gas supply reaches approximately 400 psig, it can be secured and the other supply opened.

By keeping the system set-up in this manner, the depleted cylinder(s) can then be changed out, and a full cylinder placed in the ready, without interruption of breathing air. Prior to attaching the cylinders, each HP circuit should be inspected, for signs of damage.

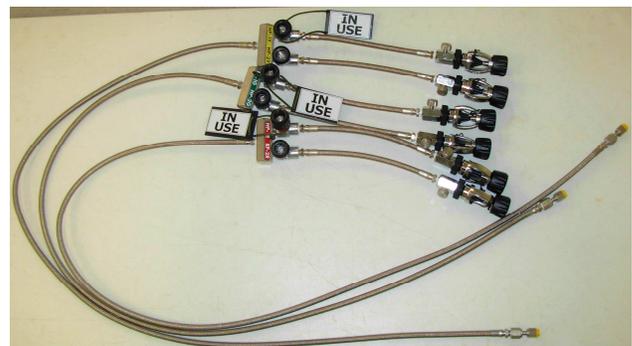

HP Whip Assembly - 3 Diver

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

General Cleaning/Inspection Procedures

Prior to commencement of system work, a clean area should be established and tools to be used must be clean and free of grease and oil. Persons performing repairs and overhauls should be trained and experienced.

Cleaning Solution

All components of the XLDS and RDC should be cleaned using a detergent like Simple Green diluted, with clean filtered water at a ratio of 1 and 1/2 ounces of detergent to each gallon of water. Regular hand washing type dish detergent, or Non-Ionic Detergent may also be used by mixing at a ratio of, one tea spoon per gallon of water. All components must be thoroughly rinsed with fresh water. After rinsing, take a sample of the final rinse water in a clear container and perform a shake test to check for suds, re-rinse components if suds are observed during shake test.

Corrosion

Parts showing corrosion should be cleaned with detergent and water to remove as much old lubricant as possible, and then acid cleaned by immersion in a 50/50 solution of white vinegar and water for up to 4 hrs. Re-clean parts using the detergent solution and rinse thoroughly.

Inspection

After cleaning, the parts should be inspected for obvious contamination and re-cleaned as necessary and carefully inspected for signs of wear and damage.

Drying

All parts should be left to air dry in a clean controlled space, or dried using nitrogen or divers' air. A hair dryer set on a low heat is also an

effective way of drying parts. When parts are dry, inspect using a bright light. Complete a final visual inspection and if any contamination is found, the components must be re-cleaned.

Control of Cleaned Components

All parts cleaned should be protected by sealed airtight designated containers or individually bagged as necessary until reinstalled in the system. All attempts should be made to maintain Foreign Material Exclusion (FME) of all parts and components, during all phases of the repair/overhaul process.

Cleaning and Handling of O-rings

All O-rings used in the XLDS and RDC will be cleaned using a detergent solution then thoroughly rinsed, dried and sealed, in an appropriate container. Once cleaned, all O-rings should only be handled while wearing gloves. O-rings should not be lubricated, until they are staged, and ready to be installed into the components.

Lubrication

Lubricant applied to O-rings and components, must be done sparingly. The recommended lubricant is Christo-Lube® or Tribolube®.

Pipe Threads

Pipe thread fittings in high- and low-pressure breathing gas systems, are often used as an alternative to straight thread O-ring or welded fittings due to cost, complexity, and selection.

Pipe thread fittings offer an attractive alternative to large bend radius welded, or compression joint systems, and can produce exceptionally strong, reliable, compact systems.

However, shock and vibration especially in portable systems can cause movement between joints resulting in leaks. Unlike O-Ring fittings,

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

minor pipe thread fitting leaks will not suddenly or drastically increase because of the natural locking nature of pipe threads. Teflon tape is used both as a lubricant and a sealant. As a lubricant, the tape keeps the threads from galling. As a sealant, the tape produces a gas tight seal. Unlike pipe fittings, minor Leaks in O-Ring fittings cannot be tolerated, because the seal is made by the O-Ring only, between two surfaces and leakage will normally increase rapidly especially if there is any movement of the fittings. In some cases, parts of the O-Ring may extrude causing sudden massive leakage or total failure of the O-ring seal.

Unlike O-rings, the pipe threads use sealing tape which will usually show up as a minor leak and will not progress significantly as long as there is no movement of the fitting. Very minor leakage in pipe thread fittings is common, should be expected, and does not pose an operational hazard in "AIR SYSTEMS", or a significant reduction in operational capability as long as the leaks are minor and can be identified, and quantified. All leaks should be repaired as soon as possible / practical. It should be understood, that in portable fast response systems like the XLDS which can be subjected to shock and vibration during transport minor leaks may result that may have to wait before repairs can be made.

The only way to remedy leaks in pipe thread fittings, is to depressurize the system, disassemble the joint, remove old sealing tape, brush clean and inspect the threads for damage, and then re-tape and re-make the joint. Because this is often impractical to accomplish in the field, minor leakage during system use, can be an acceptable alternative to field repairs in order to safely continue with diving operations until re-sealing can be accomplished.

WARNING

Never tighten fittings or components while the system is pressurized. Attempting to tighten fittings, while the system is pressurized, could result in component failure, resulting in serious injury or death.

Checking and Quantifying Leaks

There is a full system step by step test procedure for pressure testing. XLDS RDC Console Annual Pressure/joint Tightness Testing Test which should be done annually, but can also be done at any time leakage is suspected. However, as a quick field check if necessary, complete a check as described herein to quantify leakage.

Checking for Leaks Quick Check: To check for leaks, ensure the umbilical supply valves, pneumofathometer valves, and cross connect valves are shut, then slowly open each cylinder HP supply valve, and each supply block valve approximately 1/4 -1/2 turn, and pressurize each HP circuit, using at least a 3000 PSIG supply pressure. Load each regulator to 350-400 PSIG and allow the system to settle for at least one minute then secure the cylinder valves only, then record the high and low pressures and the time. Allow the system to sit for ten minutes, then check the gauges. If there has been any loss of pressure, apply soapy water solution to all joints and fittings to identify the leaks. Very minor leaks at pipe threaded joints, that cause a drop of gauge pressure of no more than 10 PSIG in ten minutes, with the supply isolated at the HP blocks as noted on each of the high-pressure gauges, do not require immediate re-sealing. Pressure loss in excess of 10 PSIG, represents a gas loss in excess of 3 liters in ten minutes, and should be corrected before the system is used. This leakage is

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

acceptable for pipe thread fittings and joints only, O-ring and or any other types of leakage must be repaired prior to use. Use the Dive Lab Appendix A2.1A Pressure/Joint Tightness procedure.

NOTICE

The purpose for the allowable leakage, is to allow continued use of the system to be used, until repairs can be made.

Teflon Tape

When making up pipe fittings of 1/4" or smaller, for best results, use three (3) mil thickness Teflon® tape. The tape used should be 1/4" wide. Half inch (1/2") wide, three (3) mil tape on 1/4" or smaller pipe threads, can be used but will not stretch and form to the small diameter threads, as well as 1/4" tape. Normally, 1-1/2 wraps applied under tension, is all that is required on brass to brass fittings, however for stainless fittings we recommend up to two and a half (2-1/2) wraps to achieve a tight seal. The tape should be applied under tension, starting 1-1/2 to 2 threads back, from the start of the fitting. In addition, we recommend applying a small amount of Christ Lube over the Teflon® tape.

Making up 3/8" to 1/2" Pipe Fittings

When making up three eighths (3/8"), or half inch (1/2") pipe fittings, three (3) mil thickness Teflon tape, or six (6) mil thickness tape, half inch (1/2") wide may be used. If three (3) mil is used, use two (3) to four (4) wraps. If six (6) mil is used, use one and a half (1-1/2) to two (2) wraps. Apply tape under tension starting one and a half (1-1/2) to two (2) threads back from the start of the threads.

Torque/Tightening

Pipe threads should be tightened using good engineering practice. Tighten pipe threads securely, but do not over tighten. Normally pipe

threads should engage at least 1 ½ to 2 full turns by hand, followed by at least 2 full turns by wrench.

RDC Regulator

The standard regulators used for the RDC, are Aqua Environments® model 873-400 piston type hand loaded, self-venting regulator of a balanced poppet design which delivers high flow with a minimum effect on outlet pressure. The poppet assembly is contained in a cartridge, with internal filtration for easy in-field changing. The regulator is NOT intended for oxygen, or oxygen enriched gas mixtures. The regulator should be used with filtered, breathing quality air only.

Specifications

- Maximum inlet pressure 5000 PSIG (340 BAR)
- Outlet pressure 0 - 400 PSIG
- Flow coefficient (Cv) 0.8 (equivalent to 0.23" orifice)
- Rise of outlet pressure with drop of inlet pressure 10 PSIG/1000 PSIG
- Materials – body and cap – aluminum
- Internals – brass, stainless
- Seals – KEL-F, Buna, Viton
- Fittings – ¼" FNPT inlet
½" FNPT outlet
- Size – 3" dia. x 6" long

Installation

Use only Teflon® tape on inlet and outlet threads of the aluminum regulators never use lubricant on aluminum threads used in high pressure piping systems. Avoid over tightening of pipe threads. Pipe thread fittings should thread in approximately 1 ½ to 2 threads by hand, and 2 threads by wrench. Normal torque, applied with an 8-12 inch long wrench, is ample.

The inlet (HP) is on the left, when facing the adjusting knob with the two gauge ports upward.

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

The ½" port is the outlet. The ¼" port adjacent to the ½" port, is the LP that is plugged with a pipe plug. The port to the left is a HP outlet port and is also plugged.

The HP inlet port is directly on the opposite side of the regulator body, opposite the large ½" port.

CAUTION

An outlet gauge and relief valve set no higher than 280 psig

Operation

Outlet pressure is adjusted by rotating the regulator hand wheel, to the desired value, as read on the outlet gauge. When reducing the pressure, the regulator will not vent the LP manifold, because of the check valve at the outlet of the regulator. It will vent slightly, when first backed off via the vent hole near the cap. This is normal. To lower the manifold pressure, vent the umbilical pressure to below the new setting, then increase pressure to the new setting.



Figure 1

CAUTION

Maintenance and Repair

As with any regulator or valve, particulates or moisture, can plug or freeze the internal filter or valve seat. This can occur, when air compressor supply dryers are not adequate, or are not used regularly. The regulator should be overhauled, at least every five years. Systems in continuous use, may require overhaul more often. The user should establish time intervals for changing the valve cartridge, filter, and any upstream dryers, based on experience and service conditions. Back-up systems should be used in very critical applications, since field maintenance is hard to ensure. The poppet cartridge (2) is a factory assembled item, and should be replaced as an assembly. Always keep at least one spare cartridge on hand for repairs. In all cases, the unit can be returned to Dive Lab for repair. Maintenance or repairs, should only be done by qualified personnel, using the information and procedures and

Trouble Shooting

The number one cause of leakage in the high-pressure regulator, is a dirty corroded HP seat, due to dirt or moisture in the air supply. If leakage occurs through the regulator, or out the regulator vent, allow the inlet and outlet pressure, to equalize by shutting off the inlet. If leakage continues after the inlet and outlet equalize, the vent seat (8) or piston seal (6) is leaking. Replace both. If leakage stops, when the inlet and outlet pressure equalize, the poppet cartridge item (2) is leaking. Replace. Consult Dive Lab, if necessary.

NOTICE

Overhaul of the regulator should be limited to cleaning and changing the HP cartridge assembly as well as the upper piston assembly.

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

Regulator Overhaul

1. Do not use silicone or Christo Lube, on threaded high, or low-pressure inlet outlet fittings. Use Christo Lube MCG 121 on O-rings, on the bearing (13) and (12), and on threads between items (16) and (17), and between (1) and (18).
2. The regulator internal components, can be overhauled, with the bottom end of the regulator in place. The regulator bottom, need not, be removed from the system.
3. Remove the regulator adjustment knob (15) and stem (16), as an assembly.



Figure 2

4. Apply several wraps of electrician's tape or equivalent, around the upper housing (18) to prevent scratching, then using a "clean dedicated" oil filter wrench, to loosen the upper body (18), then remove by hand.

NOTICE

Aqua Environments regulators made after 2015 have a small hole on each side of the regulator body, to allow for using a spanner wrench instead of an oil filter wrench.



Figure 3



Figure 4

5. Remove items (14), (12), (13), (10), (11), as a stack, place these items in a small, clean container.

NOTICE

The above items are outside of the breathing air system. If the items show no signs of dirt and corrosion, cleaning is not required. If in doubt, clean and re-lubricate with Christo lube, or food grade Silicone grease.



Figure 5

6. Carefully remove the piston housing, clean and inspect all components. Lightly lubricate new O-rings on new service kit. Figure 6.

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL



Figure 6

7. Remove low pressure piston assembly.



Figure 7

8. Remove high pressure valve assembly, in regulator body.



Figure 8

9. Inspect regulator body for damage and/or corrosion. If nothing found install new kit.

NOTICE

If the housing is heavily corroded, remove it in accordance with the procedures, listed in the one-way valve removal section.

10. Install NEW high-pressure valve assembly, in regulator body. Tighten to 80-100 inch lbs.



Figure 9

11. Install NEW low pressure piston assembly.



Figure 10

NOTICE

Packing the vent seat area with Christo Lube, is done to secure the seat during assembly.



Figure 11

4. Lay the stop ring (9) down on top of the lower regulator body (1) as shown so the bevel is down, see Figure 13 & 14. Carefully place the piston housing assembly over the bevel ring into place. Use care not to drop the seat.

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL



Figure 12



Figure 13

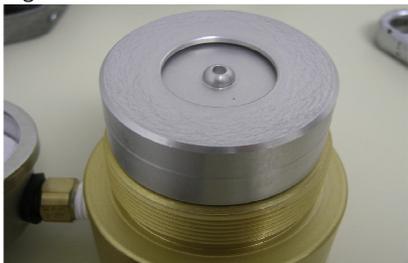


Figure 14

5. Lubricate, then stack the following items: Spring Pad (11), Spring (10), Brass Washer (14), SS Washer (12), Bearing (13), SS Washer (12), Brass Washer (14).

NOTICE

Make sure the top washer (14), has the tapered hole bevel facing up, for smooth engagement to the stem (16).



Figure 15

6. Ensure the lower body threads have been lightly lubricated, then carefully load the top of the body, down onto the lower body snug with moderate force, using the oil filter wrench.
7. Liberally lubricate the end of the stem (16), as well as the threads, and secure into the top of the body.

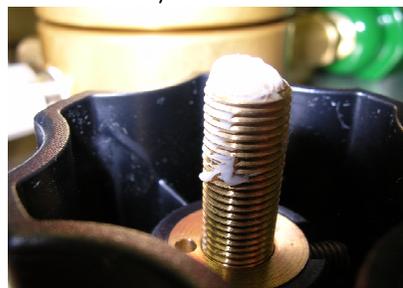


Figure 16

8. The regulator should now be tested for proper operation.

Low Pressure Umbilical Supply Valves / Cross-Connect Valves Overhaul

The quarter turn valves used for the LP cross connect and umbilical supply are very reliable and require only minimal maintenance.

All valves are made of 316 stainless steel, and have a rated working pressure for the XLDS of 400 psig. The valve should be overhauled at least every five years, or whenever the valve does not operate smoothly, or if any leakage occurs. The valve is simple to disassemble and service, however, the person performing service must be knowledgeable and properly trained. The cross-connect valve and the umbilical supply valve, use the same components, except for the nylon locking nuts. Overhaul is done in the same manner.

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

Preliminary

Ensure all high-pressure gas supplies have been disconnected, and all pressure has been vented. Open each diver circuit pneumofathometer valve, to ensure the system is vented, then open each umbilical supply valve. Ensure the work area and all tools are clean.

The two and three diver RDC units are disassembled and reassembled in the same manner, therefore, this procedure will work for both with only minor variation. It is strongly recommended that you take pictures of pneumo hose routing.

Tools and Components Needed

3/8" Open End Wrench
9/16" Open End Wrench
1/2" Open End Wrench
Torque Wrench 0-250 inch lbs.
3/8" Socket short
7/16 Socket
9/16 Socket
1/2" Socket
Christo Lube®
Overhaul Kit PN# 1XL8RK
Brass Pick Set
Needle Nose Pliers
Thread Locker Compound-Medium Strength

NOTICE

Removing the entire manifold system from the foundation plate (1), allows easier access to the valves. Removing the entire manifold system, is very quick and easy.

1. Loosen and remove the hose fittings on Green, Red and Yellow divers' pneumofathometer valves (11).



Figure 17

2. Loosen and remove all the 7/16" lock nuts, from each of the clamp blocks (21), then remove the blocks and rubber strips. There are 8 blocks on the three diver, and 5 blocks on the two diver consoles.



Figure 18

3. Lift the two or three diver manifold assembly from the box, as a whole. Place the manifold on a clean flat work table.



Figure 19

4. Using the 1/2" wrench, loosen then remove the valve handle retaining nut (12), from each valve being disassembled, then remove the lock washer (13) and handle (11).

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL



Figure 20

- Using the 9/16" wrench, loosen then remove stem cap (7) from each valve.

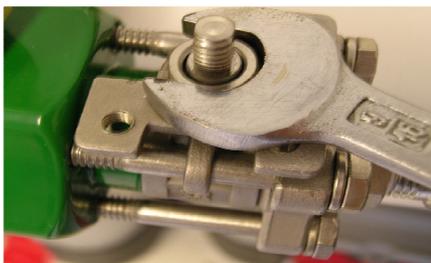


Figure 21

- If the cross connect valves are being serviced, loosen and remove the 4 bolts (9) and nuts (10). If the umbilical supply valves are being serviced, remove the bolts and nut (25).



Figure 22

- Remove the center section (1).



Figure 23

- Press in on one side of the ball until one of the plastic end seals (6), until the other pops free, then rotate the ball (5), until the slot is parallel, with the center section then, the ball will fall free.

NOTICE

Take care not to scratch the ball. If the ball is scratched, it will not seal and must be replaced.



Figure 24

- Push down on the stem shaft (40), and work to one side, until it pulls free, then remove the old stem washer (3).



Figure 25

- Using a brass pick from the outside of the valve, pull up and remove, the two white packing discs (2) rings and discard.

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL



Figure 26

11. Clean and inspect the ball (5), stem (4), stem cap (7) and center body section (1). If the Ball (5), center section (1) or stem (4) shows signs of damage from scratching, pitting, corrosion or wear, replace the complete center section.
12. Apply a light coat of Christo Lube® on the exterior of the new packing, and insert the packing into the valve center body (1).
13. Lightly lubricate the stem shaft, then install the Teflon® stem washer (3), then slide the valve stem (4), up into the new packing (2), from inside the valve center body (1). Make sure it is pressed all the way up, into place.



Figure 27

14. Install the stem cap (7), hand tight only.

NOTICE

Make sure the ball is located in the fully closed position before tightening the four bolts.

15. Install the ball (5), so the groove is centered with the stem, then lightly lubricate the white plastic ball seals (6), and install with the concave sides in, against the ball. Ensure the plastic seals are properly seated. Make sure the ball is in the fully closed position.

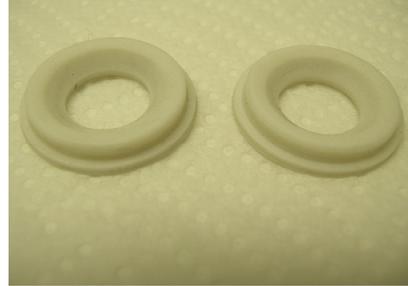


Figure 28

16. If the valve is an umbilical outlet valve ALP-1R, ALP-2G, ALP-3Y, apply a drop of thread medium or low setting thread locking compound to each bolt, at the start of the thread, then install the lock-washers and bolts (25, 27), and slowly draw up, evenly tighten in an X pattern into the end of the manifold, in three steps 10 inch lbs., 30 inch lbs., and finally torque to 60 inch lbs.

NOTICE

If the valve was a cross connect valve, reinstall the 4 bolts (9), so that the head of the bolt faces green diver manifold.

Install the lock nuts (10), lightly tighten using an X pattern 180°aparting, then torque to 60 inch lbs.

17. Torque stem cap (7) to 60 inch lbs., operate the stem with the handle several times, to ensure smooth operation, then re-torque to 60 inch lbs.

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL



Figure 29

18. Re-install the manifold in the box, making sure each clamp block, has the rubber strip installed. Tighten all clamp blocks to 40 inch lbs.
19. Reinstall the pneumofathometer fitting to each pneumo valve, and lightly tighten.
20. Perform a pressure test of the LP system.

Check Valve / One Way Valve

Each regulator is attached to the manifold, via a 1/2" brass male pipe thread (MPT), one-way valve. This same valve with a 1/2" elbow, can also be installed on the manifolds, for use if an LP supply is to be used. The one-way valves should be disassembled, inspected, and cleaned, and the sealing O-ring (5), at least every 5 years if the console is being used with HP air only, and once a year, if used with LP compressors, or whenever the valve fails a sealing/leak test.

Overhaul of the valve is limited to cleaning the body, spring and poppet, and replacing the O-ring (5).

NOTICE

The valve body need not be removed, unless it is severely corroded, contaminated or damaged. To remove the body, use a 12 inch long piece of PVC pipe 3" diameter, to hold the regulator body, and a 7/8" open end wrench, to turn the one-way valve body.

CAUTION

The threads that join the two halves of the one-way valve body, should not be over-tightened. The valve body halves, should be tightened to between 100-120 inch lbs.

Tools and Materials Needed

7/16" Socket
5/8" Open End Wrench
7/8" Wrench (2)
Torque Wrench 0-250 inch lbs.
Torque Wrench Crows Foot Adapters
3/8" Socket Short
Christo Lube®
O-Ring PN# 1XL25R
Brass Pick
Needle Nose Pliers
Flashlight
3" Diameter 12 Inch Long Piece of PVC Pipe
(used as a Regulator Holder)
3/4"-1" Tube Brush

Preliminary

To remove the valve from the manifold and regulator, the complete manifold system must be unbolted from the foundation plate (1), and removed from the console.

Ensure the work area and all tools are clean. Ensure the gas supplies have been disconnected, and all pressure has been vented. Open each diver circuit pneumofathometer valve, to ensure the system is vented. The two and three diver RDC units are disassembled, and reassembled in the same manner, so this procedure will work for both with only minor variation.

1. Loosen and remove the hose fittings on Green, Red, and Yellow Diver pneumofathometer valve (11).
(Same picture as the three way valve).

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL



Figure 30

2. Loosen and remove all the 7/16" lock nuts, from each of the clamp blocks, then remove the blocks and rubber strips. There are 8 blocks on the three diver, and 5 blocks on the two diver consoles.



Figure 31

3. Lift the complete two, or three diver manifold assembly from the box as an assembly. Place the manifold on a clean, flat, work table then remove the hand loader knobs.



Figure 32

4. Position the regulators, so they hang over the edge of the work bench, and using two 7/8" wrenches, loosen and separate, the one-way valve, by turning counter - clockwise.

NOTICE

Use care when separating the valve, so the spring and poppet don't fall free.



Figure 33

5. Remove the spring (3), and poppet/spring housing (2), then using the flashlight, carefully inspect the insides of each half, for corrosion and contamination.

NOTICE

Remove the O-ring using a brass, or plastic pick only. The use of steel picks or screw drivers could scratch the seat, causing the valve to leak.



Figure 34

6. Using the brass pick, remove the O-ring (5).

NOTICE

If the body (4), spring (3), and poppet/spring housing (2), are clean and free of corrosion, cleaning will not be necessary, and simply lubricating and installing the new O-ring, is all that is required. Skip steps 7 and 8 and continue to step 9.

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL



Figure 35

- Using 12" long piece of 3" diameter plastic (PVC) pipe, hold the regulator, while turning the check valve body counter-clockwise, with the 7/8" wrench.



Figure 36

- Using a 7/8" wrench, while securely holding the manifold assembly, remove the other half of the one-way body, from the manifold, by rotating it counter-clockwise.



Figure 37

- Using the tube brush and detergent solution, carefully clean the interior surfaces. After cleaning, inspect for corrosion, and soak if necessary in a 50/50 solution, of vinegar and water.

- After cleaning, rinsing, and drying the body, inspect using a bright light for damage in the form of pitting or galling. Check the spring for corrosion. If the valve shows any signs of damage, replace the entire valve.
- Lightly lubricate the new O-ring (5), and install in the regulator side of the body, use the poppet as a tool, to position the O-ring into place, then load the poppet/spring housing (2), and spring into place, and carefully re-connect, the two valve body halves. If the entire valve assembly had been removed, reassemble, then re-tape each end and thread into the manifold first but only lightly tighten, then install the regulator body hand tight.
- Install the PVC pipe over the regulator, and using the 7/8" inch wrench, loosen the two valve halves. Tighten the regulator side of the valve until almost tight, then tighten the valve halves to check for alignment.
- After checking alignment, alternate the tightening of the valve body halves, until the regulator is upright and level, and the joints are tight.
- After all manifold repairs have been made, load the manifold assembly back onto the foundation plate, replace all rubber strips and securing blocks, then tighten all nylon nuts to 30 inch lbs.
- Reinstall the pneumofathometer hoses, and tighten, using good engineering practice.
- Perform a leak check, by pressurizing the low pressure system, to at least 350 psig, and then secure and bleed down the high-pressure supply system. The low-pressure circuit should lose 10-20 psig, as the one-way

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

valve shuts, and then should hold pressure with no leakage, hold for at least 5 minutes.

Pneumofathometer Valve Lubrication

Preliminary

There are two types of Pneumofathometer valves, that have been used on the XLDS. On units made prior to 2010, a brass Hylock® angle valve, with a metal to metal seat was used. On units made after 2011, a stainless steel Hylock valve was used, which employs a soft seat stem. These valves will operate for many years and require lubrication only once a year. If repair is needed the repair is limited to replacement of the packing, and stem only. The valve can be sent to Dive Lab, for a complete overhaul, if necessary.

NOTICE

The two and three diver RDC units use the same model valve, and are disassembled and reassembled in the same manner.

Tools and Components Needed

9/16" Open End Wrench
5/8" Open End Wrench
Torque Wrench 0-250 inch lbs.
5/8" Crow Foot Adapter for the Torque Wrench
11/16" Open End Wrench
8-10" Adjustable Wrench
3/32" Allen Wrench
10x Magnifying Glass
Teflon Tape
Christo Lube
Lint Free Cloth

1. Disconnect all gas supplies. Ensure the system is vented and the LP gauges read zero.

2. Using the 5/8" wrench, loosen and remove the bonnet nut (3), by rotating counter-clockwise.



Figure 38

3. Unscrew (back out) the valve handle counter-clockwise, and pull the knob (8), and stem (4) free.



Figure 39

4. Inspect the seat area in the valve for damage, corrosion and contamination. If the valve is free of corrosion and damage, wipe the threads of the stem (4), clean with a clean lint free cloth, lightly lubricate the stem threads, and packing area with Christo Lube®, and reinstall into the body.

NOTICE

Thread stem (4) in, by hand lightly, until it bottoms out, then engage the bonnet packing nut (3), and hand tighten only at this time.

5. Back the stem out one to two turns, then torque the packing nut (3) to 15-20 inch lbs.
6. Test operate the valve without pressure, then

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

perform a seat tightness test by installing the valve back in the system and loading the regulator to 350 psig, then checking the discharge end of the pneumofathometer fitting for leaks, by placing the end of the QD fitting in a glass of clean fresh water, for at least one minute, to check for bubbles.

Replacing the Valve Packing / Stem

1. In the unlikely event, the valve packing and or stem need to be replaced, ensure the system is depressurized, remove the valve knob (8), using the 3/32" Allen wrench, remove the knob set screw (8), and knob (7).
2. Loosen and remove the bonnet nut (6).
3. Remove the stem (2).
4. Remove the spacer (5), plastic packing (4), and washer (3), then wipe the stem clean, and inspect for damage in the form of scratches, corrosion and damaged threads. Replace the entire valve stem, if the stem is damaged. Look down into the valve body (1), for signs of damage. If the valve stem seating area shows any damage, the entire valve assembly should be replaced.

Reassembly

5. Lightly lubricate the stem shaft and threads, then install the washer (3), the plastic packing (4), then the spacer (5).
6. Thread stem (2) in by hand lightly, until it bottoms out, then engage the bonnet packing nut (6), and hand tighten only at this time.
7. Back the stem out one to two turns, then torque the packing nut with the 9/16" adapter to 50 inch lbs., to set the packing, then loosen and re-torque to 25 inch lbs.

8. The valve should be tested after any work is done. Ensure the valve is shut, then load the regulator to 350 psig, and check the discharge end at the female QD fitting for leaks by placing the open end of the QD, in a glass of water for at least one minute, to check for bubbles.

Removing / Replacing Pneumo Valve

1. Using a 9/16" open-end wrench, remove the pneumofathometer supply hose, for the valve being removed.
2. Using the 11/16" open end wrench on the valve body, remove the valve by turning counter-clockwise.

New Valve Installation

1. Tape the end of the valve with Teflon tape. Starting two threads back apply 2 full wraps.
2. Ensure the threads in the manifold are clean of old Teflon tape, and the threads are not galled or damaged, then install the pneumo body, and tighten securely using an open end 11/16 wrench ensuring proper alignment, for the hose and fitting.
3. Re-Install the hose and tighten, using a 9/16 open end wrench. Torque the hose fitting to 50-inch /lbs.
4. Check the valve for seat tightness and leaks, by first closing the valve, then slowly load the regulator to 350 psig.
5. Place the open end of the QD fitting in a glass of water, to check for seat leaks, for at least one minute.

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

High Pressure Supply Valve Overhaul

There are two types of high-pressure supply valves that have been used on the Dive Lab HP routing blocks. All systems made before January of 2012 used Sherwood® line valves, model #YVA3010. After 2012, Thermo® line valves became standard. See Figure 40.



Figure 40 Thermo & Sherwood Line Valves

Disassembly and assembly procedures are the same for both valves. These valves are normally used for high-pressure air transfer systems, and are durable, reliable, and require minimal service. Overhaul of the valve is limited, to replacing the sealing washer (20), soft seat (3), stem packing (5). The valve should be overhauled at least every five years, and/or whenever damage or wear is suspected/found, or if the valve does not operate properly.



Figure 40-1 **Top:** Sherwood Valves Exploded View
Bottom: Thermo Valves Exploded View

NOTICE

The valve can be disassembled in place, and does not require removal from the block and hose, providing the valve body and internal body seat, does not show signs of contamination, and/or damage.

Preliminary

1. Ensure the HP supply whips are disconnected from the cylinders, and the system has been vented.
2. Open both HP valves, HP-1, HP-2.
3. Ensure the work area is clean, and all tools are clean.

Tools and Components needed

- 10" or Large Adjustable Wrench Or Vice
- 0-250 inch lbs. Torque Wrench
- 11/16" Open end Wrench
- 11/16" Crows Foot Adapter
- 1/4 " Tube Brush
- 10x Magnifying Glass
- Brass Pick
- ¼-3/8" Flat Blade Screwdriver
- Christo Lube
- Soft Good Kit PN#3XL89RK

Disassembly

1. Open the valve being serviced fully, counterclockwise.
2. Remove the slotted retaining nut (10).



Figure 41

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

3. Remove the spring (9).



Figure 42

4. Holding the valve body (1), in a vice or with the adjustable wrench, loosen the bonnet packing nut (7), by turning counter-clockwise, then remove with the stem (3).



Figure 43

5. Rotate the soft seat (5) counter-clockwise and remove.



Figure 44

6. Using the brass pick, remove the copper sealing washer (2).

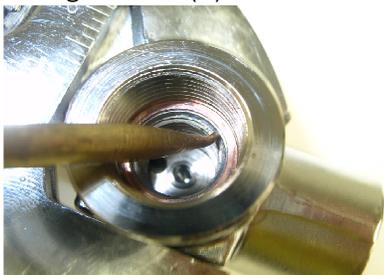


Figure 45

7. Using the pick, remove thin packing washer (4), packing (6), and discard.



Figure 46

Cleaning and Inspection

NOTICE

If the valve body shows signs of corrosion and or contamination, the valve should be removed from the HP block, and the HP hose for cleaning.

CAUTION

Use care, not to scratch the valve body seat area, when cleaning.

1. Place the valve body, and all valve components, in a solution of detergent and warm water, and carefully clean with the tube brush. Corroded parts should be soaked in a 50/50 solution of vinegar, and water for 1–3 hours, then re-clean, thoroughly rinse, and inspect for corrosion and damage. If the body or stem, shows any signs of damage, the entire valve should be replaced.

NOTICE

Lubrication should be done sparingly, on the stem shaft, and packing nut threads only.

2. After all interior and exterior surfaces have been cleaned, dried and inspected, install the

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

new seat (5), and thread it all the way down, using the flat blade screw driver.

3. Install the thin copper washer (2), in the body.
4. After inspecting the stem, lightly lubricate the stem shaft (3), then install the new washer (4), packing (6), into the packing nut (7), apply a small amount of Christo lube on the packing nut threads.



Figure 47

5. Engage the cap nut (7) threads into the body (1), and lightly turn the stem, until it engages the slot in the soft seat. Then tighten the bonnet nut by hand, until it bottoms out.



Figure 48

6. Back out one-two turns counterclockwise on the stem, then using the torque wrench, torque the packing nut (7) to 150 inch lbs.



Figure 49

7. Place the knob (8) on the stem, and rotate the valve shut. Then pull the knob off, leaving the stem and packing nut visually exposed.



Figure 50

8. Perform a leak test on the valve, using full system pressure. The simplest test, is to shut both valves on the HP block, attach HP supply gas to the valve to be tested, and slowly pressurize to the maximum HP supply pressure, 4350 psig for DIN and 3500 psig for "A" Yokes.

At the same time, spray the valve stem and packing nut, with soapy water to identify any packing leaks. Hold test pressure for at least one minute. If any leakage is found, repair or replace the valve.

9. Upon successful test, install the knob (8), spring (9), and retaining nut (10), then tighten the retaining nut, until the slot is flush, with the end of the stem.

Relief Valve Cleaning Inspection and Overhaul

The Relief valve used in all RDC units, purchased before 2011, is the Circle Seal® 0-400 psig, adjustable brass body relief. RDC consoles sold after 2011, use the Hylock SS angle relief. Both valves are very rugged and dependable, and can be easily serviced by trained persons. Dive Lab strongly recommends, only factory trained technicians service this component. Overhaul is limited to cleaning and replacing the soft seat. If

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

any other damage is found, the valve should be replaced. The following procedure covers overhaul of the Circle seal valve, followed by the overhaul procedure for the Hylock SS angle relief.



Figure 51 (Old Relief PN# 1XL7-4RK)

NOTICE

The valve can be disassembled in place, and does not require removal from the manifold block, providing the valve does not show signs of contamination, corrosion and /or damage.

Preliminary

1. Ensure the HP supply whips are disconnected from the cylinders, and the system has been vented.
2. Ensure the work area is clean, and all tools are clean.

Tools and components needed

- 1" Open End Wrench (2 each)
- 0-250 inch lbs. Torque Wrench
- 5/16" Allen Wrench
- 1/16" Allen Wrench
- Needle Nose Pliers
- 10x Magnifying Glass
- Brass Pick
- Small Blade Pocket Knife or Exacto Knife
- Christo Lube
- New O-Ring PN# 1XL7-4RK
- Flashlight

- Nylon Tooth Brush
- Tweezers
- Low Lint Rags/Wipes
- Loctite® 222

Disassembly and overhaul in place

1. Using one of the 1" inch wrenches to hold the base of the valve, loosen the cap (9).



Figure 52

2. Using the 5/16" Allen wrench, loosen and remove the spring housing (8), spring (7), spring pad (6), seat assembly (2, 3, 4, 5).



Figure 53



Figure 54

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL



Figure 55

3. Inspect all components for contamination, corrosion and damage. If the internal and external body shows corrosion or appears contaminated, remove for cleaning and further inspection, using the 1" wrench on the base of the body.
4. Using the 1/16" Allen wrench, loosen and remove the set screw (2), then unscrew the seat guide (3), from the pad guide (5), counter- clockwise.
5. Using the brass pick, remove the O-ring (4), and discard.



Figure 56

6. Place all components in a clean container of detergent and water, and clean using the nylon brush, then rinse and dry. After cleaning, inspect for corrosion and damage, re-clean as necessary. Pay particular attention to the seat area in the valve body. Any nicks or dings in this area, will cause valve leakage.
7. Replace any components in question or the entire valve.

Reassembly

1. Lightly lubricate a new O-ring (4), then place in the pad guide (5), then assemble the pad guide, seat guide together and secure.

NOTICE

The O-ring (4), is the seat material that makes the seal against the seat, in the main body. The O-ring is captured between items 2 and 4.

2. Apply a small amount of thread locking compound on the Allen set screw (2), and tighten snugly, while holding the pad guide (5).



Figure 57

3. Using the needle nose pliers or tweezers, install the soft seat assembly, so the stainless point end is pointing up.
4. Place the spring pad (6), so that the machined out area for the spring faces up, then install the spring (7), and thread the spring cap (8) into the valve body (1), until the threads disappear, then install the spring cap (8), and run it down until it bottoms out by hand.



Figure 58

5. Loosen the spring cap (8), about 1/8 of a turn, and slowly run the spring cap in, using the 5/16" Allen wrench, until there is about 3/16"

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

of an inch protruding through the main cap (9). The valve is now ready for adjustment.



Figure 59

Adjusting the Relief

NOTICE

The relief can be set between 250-410 psig, to accommodate different system configurations. To adjust, the relief needs to be installed in the RDC, or attached to a clean adjustable air source. This procedure uses the installed RDC regulator, to set.

1. Slowly open an HP air cylinder, approximately 1-2 turns, and pressurize the HP system.
2. Slowly bring pressure to the manifold, by rotating the regulator adjustment knob in, until the LP gauge reads the desired relief pressure setting.

NOTICE

If the relief starts venting before the desired relief setting is reached, slowly rotate the spring cap (8) clockwise, using the 5/16" Allen wrench, until the relief holds at, or just below, the desired setting. Then hand tighten the main cap (9), and back the regulator off one – two turns.

3. Slowly vent the pressure, below the desired set pressure, using the pneumo valve. Then slowly load the regulator, while watching the gauge, to determine where the relief lifts at.

4. Repeat steps 2 and 3 until the desired setting is achieved. Once adjusted, hold the spring cap with the Allen wrench, and tighten the lock nut counter-clockwise, with the 1" wrench, until snug. Tighten using the force of three fingers on the wrench. Or torque with torque wrench, to 50 inch lbs.

NOTICE

The working pressure of the LP system is well above the maximum relief setting, obtainable using this 0-410 psig relief. The system will not be damaged by setting the relief in place. The relief has been sized to more than accommodate the maximum flow, of the HP system.

Hylock SS Angle Relief Overhaul

As of January of 2011, the relief valves being installed in the XLDS RDC consoles is the Hylock® Model RV2MF SS, similar in operation and adjustment to the Circle Seal®, 0-400 psig adjustable brass body relief. This valve is very rugged and dependable, and can be easily serviced by trained persons. Dive Lab strongly recommends, only factory trained technicians service this component. Overhaul is limited to cleaning, and replacing the soft goods. If any other damage is found, the valve should be returned to Dive Lab, for repair.



Figure 60 (Hylock Angle Relief)

© Copyright 2003-2020 Dive Lab® Inc. All rights reserved.

This Guide is made available for the express use of owners and users of the Dive Lab 2 & 3 RDC systems.

This information is subject to periodic updates and changes. Always check the Dive Lab web site for the latest versions.

Document 2 & 3 RDC systems – Section Four A

Revised August 4, 2020

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

NOTICE

The relief valve can be overhauled in place, however for best results it is easiest to remove the relief valve from the manifold if performing an overhaul, so that the valve can be properly cleaned.

Preliminary

1. Ensure the HP supply whips are disconnected from the cylinders, and the entire RDC console has been vented.
2. Ensure the work area is clean, and all tools are clean.

Tools and Components Needed

- 3/4" Open end Wrench (2 Each)
- 0-250 inch lbs. Torque Wrench
- Crows Foot Wrench 3/4"
- 5/16 Allen Wrench Socket For Torque Wrench
- Needle Nose Pliers
- 10 x Magnifying Glass
- Brass Pick Set
- 1/4" Wooden Dowel or Plastic Rod (Blunt Ends)
- 3/32" Allen Wrench
- Christo Lube
- Soft Goods Kit PN# 1XL7RK
- Teflon Tape
- Flashlight

Disassembly and Overhaul

1. Using one of the 13/16 and 3/4 in wrenches,

2. Using the two 3/4" wrenches, loosen the lock nut (2), and then remove the cap (1). Then drop out the spring (3), and spring disk (4).
3. If the valve body is to be removed, remove it at this time, using the 13/16 wrench.
4. Remove the bonnet O-ring (6), and stem (8).
5. Using the brass pick, carefully fish out the O-ring (7), internal to the bonnet.

NOTICE

The O-ring can be difficult to remove and requires manipulation with the O-ring pick and the 6/32" Allen wrench from the bottom end of the bonnet.



Figure 61 Bonnet O-Ring

6. Using the 5/16 Allen wrench, loosen and remove the stem seat (9), then using the pick remove the O-ring (10), and body seat (11).
7. Discard the three old O-rings, then clean all the parts and blow or air dry. After drying, carefully inspect all components, for signs of damage and contamination. Re-clean as necessary.

Reassembly

1. Lightly lubricate the three new O-rings (10, 7, 6), and set aside.
2. Install the body seat (11), O-ring (10), then using the blunt end of the dowel, press down on the O-ring, and body seat to fully seat the O-ring around the body seat.

SECTION FOUR A: RDC REPAIR / MAINTENANCE / OVERHAUL

- Using the 5/16" Allen socket, reinstall the stem seat, then torque the stem seat to 150 inch lbs.
- Install O- ring (6) onto the bonnet (5).
- Using the 3/32" Allen wrench and the dull O- ring pick carefully install O-ring 7 into the Bonnet.
- Reinstall the HP supply whip to the manifold and line up a HP air supply of at least 500 psig, to the regulator for the circuit to be tested, and slowly open an HP air cylinder.
- Slowly bring pressure to the manifold by rotating the regulator adjustment knob clockwise (in), until the LP gauge reads the desired relief pressure setting.

NOTICE

This O-ring can be difficult to install take care not to cut the O-ring.

Work the O-ring into the groove, with the Allen wrench from the bottom of the bonnet, and with a dull O-ring pick at the groove end.

- Install the bonnet into the body, and torque to 150 inch lbs. Using the ¾ inch wrench, and crows foot with torque wrench.
- Install stem (8), and disc (4), and spring (3).
- Then install the lock nut (2) and cap (1) tighten, the cap approximately 6 turns, by hand.
- If the relief valve had been removed from the manifold, re-tape the pipe threads, reinstall and tighten using good engineering practice.

Adjusting the Relief

NOTICE

The relief can be set between 250-410 psig to accommodate different system configurations. To adjust, the relief needs to be installed in the RDC, or attached to a clean adjustable air source. This procedure uses the installed RDC regulator to set.

- Ensure the RDC regulator is backed off counter-clockwise, and all RDC valves are shut.

NOTICE

If the relief starts venting, slowly rotate the cap (1) clockwise until the relief stops venting. If the relief does not vent at the desired set pressure back off counter-clockwise on the cap until the relief starts venting at the desired pressure.

- Once the relief is set, retest, by slowly venting the manifold slightly using the pneumo valve, until the LP pressure reads 20-30 psig less than the desired set pressure. Slowly load the regulator, while watching the gauge to determine where the relief lifts. For XLDS use with the ICS and ¼" umbilicals, set the reliefs to start lifting at a pressure between 390-400 psig. For use with standard 3/8-1/2" umbilicals, set the reliefs to start relieving between 275-285 psig.
- Repeat steps 4 and 5 until the desired setting is achieved. Once adjusted, hold the spring cap with the Allen wrench, and tighten clockwise with the 1" wrench until snug.
Do Not Over Tighten!

NOTICE

The working pressure of the LP system, is well above the maximum relief setting, obtainable using this relief. The system will not be damaged by setting the relief in place. The relief has been sized to accommodate the maximum flow, of the HP system.

SECTION FOUR B: RDC REPAIR / MAINTENANCE / OVERHAUL

RDC System Pressure Gauge Comparison

RDC Gauge Comparison

Dive Lab recommends all XLDS system gauges as well as support gauges be compared at least every 24 months using certified master gauges. This includes the RDC Red, Green, and Yellow Diver HP, LP and diver pneumofathometer gauges, as well as EGS submersible pressure gauges, and any other pressure gauges used to support the system. Dive Lab strongly recommends performing the RDC gauge comparison in place if possible, using the Dive Lab Gauge Comparator System or similar clean gas system.

Performing in place gauge comparison significantly reduces the possibility of damaging gauges and fittings, and introducing system generated contamination in the form of Teflon® tape and metal particles due to component removal and re-installation. Guidance: Dive Lab Gauge comparator system manual Revision 4, 2018.

If the gauges are to be removed and sent out for comparison care must be taken to ensure the gauges are correctly removed, handled, and protected from damage and contamination. The gauge ports must be free of old Teflon® tape and particles. To help clear any debris from the system, flow air thru the manifolds and / or the pneumo “T”s after the gauges are removed to help keep the Teflon tape and foreign particles from entering the system while using a brass pic, and /or 3/8” round nylon tube brush to remove old tape. Cover all exposed ports and safeguard the system until gauges are ready for installation.

If the gauges are to be removed and sent out for comparison care must be taken to ensure the gauges are correctly removed, handled, and protected from damage and contamination. The gauge ports must be free of old Teflon® tape and particles. To help clear any debris from the system, flow air through the manifolds and / or the pneumo “T”s after the gauges are removed to help keep the Teflon tape and foreign particles from entering the system while using a brass pic, and /or 3/8” round nylon tube brush to remove old tape. Cover all exposed ports and safeguard the system until gauges are ready for installation.

Re-installation of gauges must be done carefully. The threads of the gauges must be clean and carefully wrapped with Teflon® tape two wraps, starting 1 ½ to two threads back from the end of the gauge stem. Lightly apply Christo Lube over the Teflon tape to assist in lubrication of threads during reinstallation. Install the gauges at approximately two turns by hand and two turns with a 9/16 wrench. **Do not overtighten.** Perform a Liquid leak test of all joints disturbed using detergent and water.

RDC System Pressure Test Procedure

A pressure test of the XLDS RDC with HP supply system should be completed at least once a year or whenever system tightness integrity is in question.

SECTION FOUR B: RDC REPAIR / MAINTENANCE / OVERHAUL

Pressure / Joint Tightness Testing

NOTICE

Prior to performing the pressure/joint tightness tests, ensure all the RDC gauges have been compared to master gauges of known accuracy. Ensure comparison has been properly documented using comparison test sheets.

WARNING

When performing any type of pressure tests eye protection should be worn at all time. Testing should be done in a clear secure area occupied by the test personnel only.

Perform a pressure / joint tightness test of the complete RDC and HP and LP supply systems to the maximum system pressure normally used. Document and use the Dive Lab RDC Pressure Test / Joint Tightness Test Procedure A2.1A. Perform the high pressure test using a minimum of 3000 psig, or to the maximum intended “use” supply pressure which could be as high as 3500 psig if using “A” yokes, up to 4350 psig using DIN connections, and to a maximum of 5000 psig with other properly rated fittings and supply whip components. The low-pressure circuits for Red, Green, and Yellow Diver’s should be tested using a test pressure of between 350-375psig and held for 10 minutes, zero leakage allowed as shown on the RDC HP and LP gauges. Document the testing on the XLDS RAPID Deployment console Annual Pressure /Joint Tightness Test Checklist A2.1A sheet.

RDC Annual Relief Valve Lift Check

The relief valves should be set to start relieving at a pressure of 290 psig as read on each of the diver LP gauges.

NOTICE

Early RDC’s (pre-2011) used brass Circle Seal® relief valves. XLDS systems after 2011 all have stainless steel HyLock® angle relief valve. Both models adjust in a similar fashion. Lift testing the reliefs will not damage the system and can be done on a routine basis if desired.

Brass and Stainless Versions:

1. Attach the HP supply to the circuits being tested. Slowly bring up pressure to the manifold by rotating the regulator adjustment knob clockwise (in), until the LP gauge reads the desired relief pressure setting.

NOTICE

Quite often if a relief has not been lifted for a long period, the relief may stick, and can go as high as twenty psig over the set pressure before it lifts. Lightly tapping on the top of the relief will often jog it free.

- 2a. **Brass Circle Seal Relief:** For the Brass Valve, If the relief needs to be adjusted proceed as follows, for the “Brass Relief”, loosen the cap (9) using a 1” wrench, then adjust the housing (8) with a 5/16 Allen wrench. Rotate out (counter-clockwise) to reduce the set pressure, or “in,” clockwise to increase the set pressure. Check the set pressure several times by slowly increasing the supply pressure until the relief lifts then vent off the pressure thru the pnemo valve. Then, while holding the position of the housing with the 5/16” Allen wrench, tighten the cap (9) with the force of three fingers on the wrench, or use a torque wrench and tighten to 40-50 inch lbs. Note the final lift pressure.
- 2b. **Stainless Hylock® Relief:** to adjust the relief. Use two ¾” open end wrenches, one on the locknut (1), and one on the cap (2), then loosen the locknut (2). Adjust the cap (1) by rotating out

SECTION FOUR B: RDC REPAIR / MAINTENANCE / OVERHAUL

(counter-clockwise) to reduce the set pressure, or “in,” clockwise to increase the set pressure. Check the set pressure several times by slowly increasing the supply pressure until the relief lifts then vent off the pressure thru the pnemo valve. Then, while holding the position of the housing with one $\frac{3}{4}$ ” wrench, snug the locknut (2) with the other $\frac{3}{4}$ ” wrench with the force of three fingers on the wrench, or use a torque wrench and tighten to 40-50 inch lbs. Note the final lift pressure.

End of Section Four B



Supplemental Information

RDC/XLDS O-Ring Chart

PART #	O-Ring Size	O-Ring Location
1XL15G	-013	1/2-20 Plug / Manifold 1/2-20 Plug / ICS Regulator
1XL15F	-011	3/8-24 Plug / Manifold Scuba Port Plug
1XL200	-010 V90	VCO Fitting / HP Inlet
1XL42	-110 H70	Pneumo Female QD x 1/4 FNPT / Console
1XL2-5	-111 90D	CV3-M8N-1/3-BRASS, Hylok Check Valve 1XL2
XL7A-6	-015 70D	Relief Valve
1XL7A-14	-106 90D	(Original) Relief Valve
1XL7A-8	-106 70D	Relief Valve

3XL25	-012 90D	Plug High Pressure 7/16-20 UNF/ High Pressure Junction Block
3XL29D	-112 90D	Viton / DIN Yoke

4XL62-72	-214 70D	ICS Regulator Tank
4XL62-5	-16	ICS Regulator
4XL62-10	-18	ICS Regulator
4XL62-9	-11	ICS Regulator
4XL62-28	-012	ICS Regulator
4XL62-25	-008	ICS Regulator
4XL62-24	-22	ICS Regulator
4XL62-7	-010	ICS Regulator
4XL62-16	-014 U70	Urathane / ICS Regulator
4XL80	-015 75D	Buna N / EGS Quick Connect
4XL80-2	-015	Backup Ring, Solid / EGS Quick Connect

6XL9	-112	DIN O-Ring Viton / EGS Tank Valve
6XL12	-015 90D	EGS & Sherwood Tank valve

